


# ACQCROSS™



## TRANSSEPTAL ACCESS SYSTEM

First System Cleared  
for Mechanical or RF Puncture

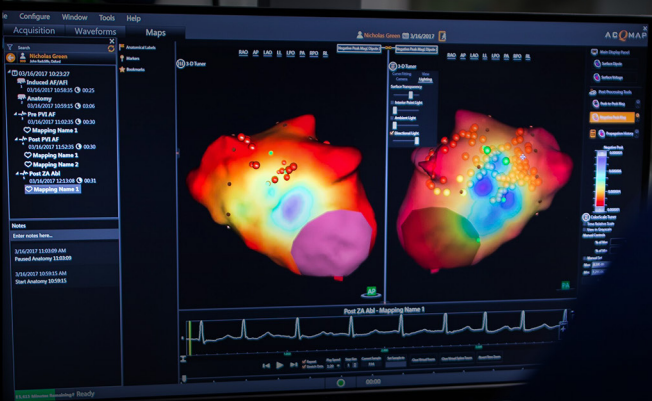

# ACUTUS™

M E D I C A L

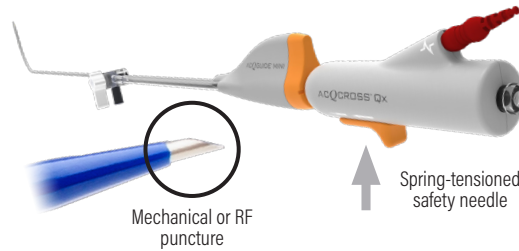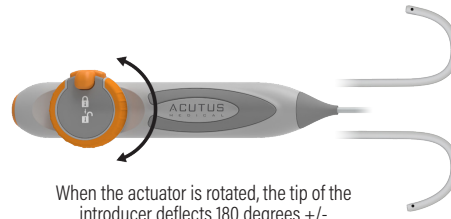

# ACQCROSS™

INTEGRATED TRANSSEPTAL  
DILATOR/NEEDLE

- Spring-tensioned safety needle; only deploys when actuated
- Integrated dilator/needle and introducer lock together as one unit for control and ease of use
- Reduce wire exchanges with retained guide-wire method
- Dual purpose needle; use mechanically or with RF energy
- Packaged as a convenient kit with Integrated dilator/needle, steerable or fixed curve introducer, guidewire, and ES and EGM cables

# ACQGUIDE™ FLEX

STEERABLE INTRODUCER


- Left-handed operation of introducer allows for simultaneous right-hand control of ablation catheters

# ACQGUIDE™ MINI


FIXED-CURVE INTRODUCER

- Facilitate positioning with fixed distal curve and improved torquability


## AcQCROSS™ Transseptal Access Procedure




**STEP 1:** Insert AcQCROSS™ Qx into Superior Vena Cava (SVC). Guidewire remains retained in dilator.




**STEP 2:** Perform 'drag-down' to locate Fossa Ovalis. Guidewire is pulled back into lumen of dilator, still retained.




**STEP 3:** Confirm correct position and tent. If repositioning is needed, re-advance guidewire back to SVC and repeat.



**STEP 4:** Needle extended and advanced into the Left Atrium (LA). Options: mechanical or RF puncture.




**STEP 5:** With needle across, advance the guidewire into the LA.




**STEP 6:** With needle safely retracted, advance AcQCROSS Qx into the LA over the guidewire.

## Traditional Transseptal Access Workflow

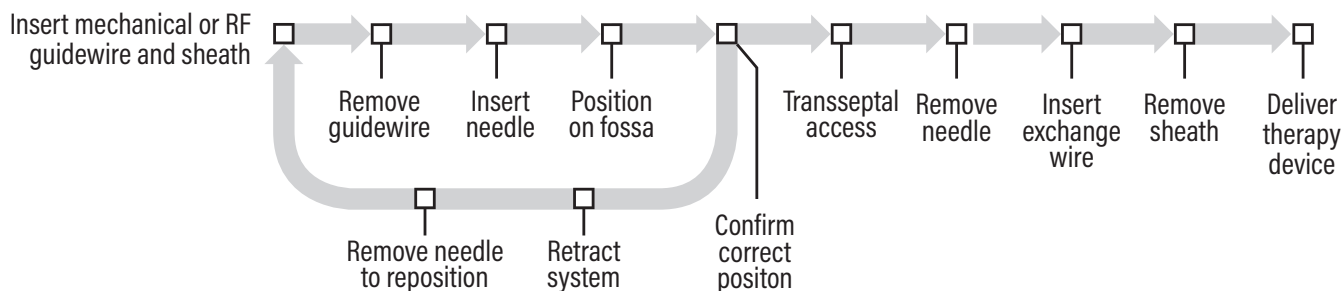

## AcQCross™ Workflow

Half the steps of a traditional transseptal access workflow

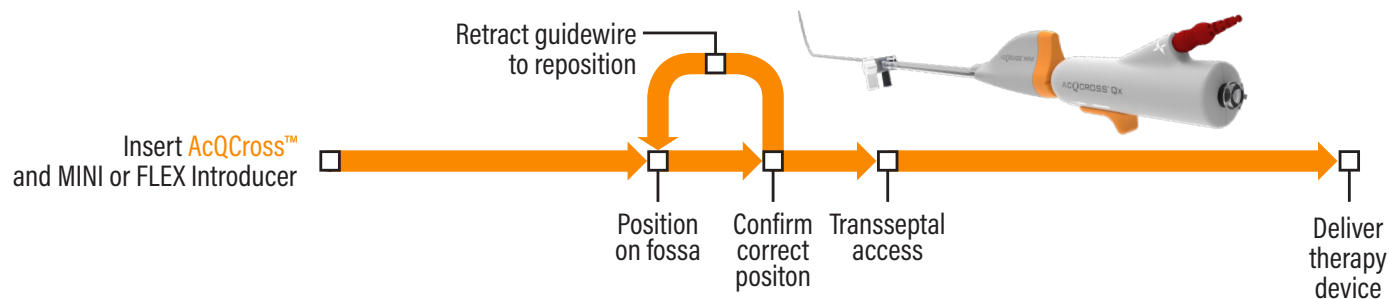

## ORDERING INFORMATION

### Transseptal Access System for Mechanical or RF Energy Application

PRODUCT NAME	PRODUCT DESCRIPTION	PRODUCT CATEGORY	ITEM #
AcQGuide® FLEX with RF 65 cm - MED Curl	65 cm, Med Curl, 8.5F ID, 12F OD	Steerable Introducer	222852
AcQGuide® MINI-S with RF 65 cm - L2	65 cm, 90 deg, 8.5F ID, 11F OD	Catheter Introducer	012852
			HCA Smart # 7350774

Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events, and directions for use. The AcQGuide® MINI with AcQCross™ and AcQGuide® FLEX with AcQCross™ devices are CE Marked and FDA cleared. [acutus.com/patents](http://acutus.com/patents)

Acutus Medical®, Acutus® and AcQMap® are registered trademarks of Acutus Medical, Inc. AcQCross™, AcQGuide® FLEX, AcQGuide® MINI are trademarks of Acutus Medical. This material is the property of Acutus Medical and its subsidiaries. Please do not copy, forward, or distribute this document. Copyright © 2021 Acutus Medical, Inc. All rights reserved.

**ACUTUS MEDICAL, INC.**  
2210 Faraday Ave, Suite 100  
Carlsbad, CA 92008 United States  
Phone: 888-202-8151  
[acutus.com](http://acutus.com)

**ACUTUS MEDICAL NV**  
Ikaroslaan 25  
1930 Zaventem, Belgium  
Phone: +32 2 669 75 00  
FAX: +32 2 669 75 01  
[acutus.com](http://acutus.com)

**ACUTUS™**  
MEDICAL

**NOTE:** All Steerable and Fixed-Curve products packaged with appropriate length AcQCross™ Qx Transseptal Dilator/Needle (8.5F OD)